


-15kV TOF: -9245 v  
 -3.6kV MCP: -3379 v  
 -2.4kV MCP: -1774 v  
 Input Cur: 298 ma  
 RPA max: 237 v  
 Mirror max: 238 v

Tue Nov 14 11:41:11 2006

## TIDE Direct Events

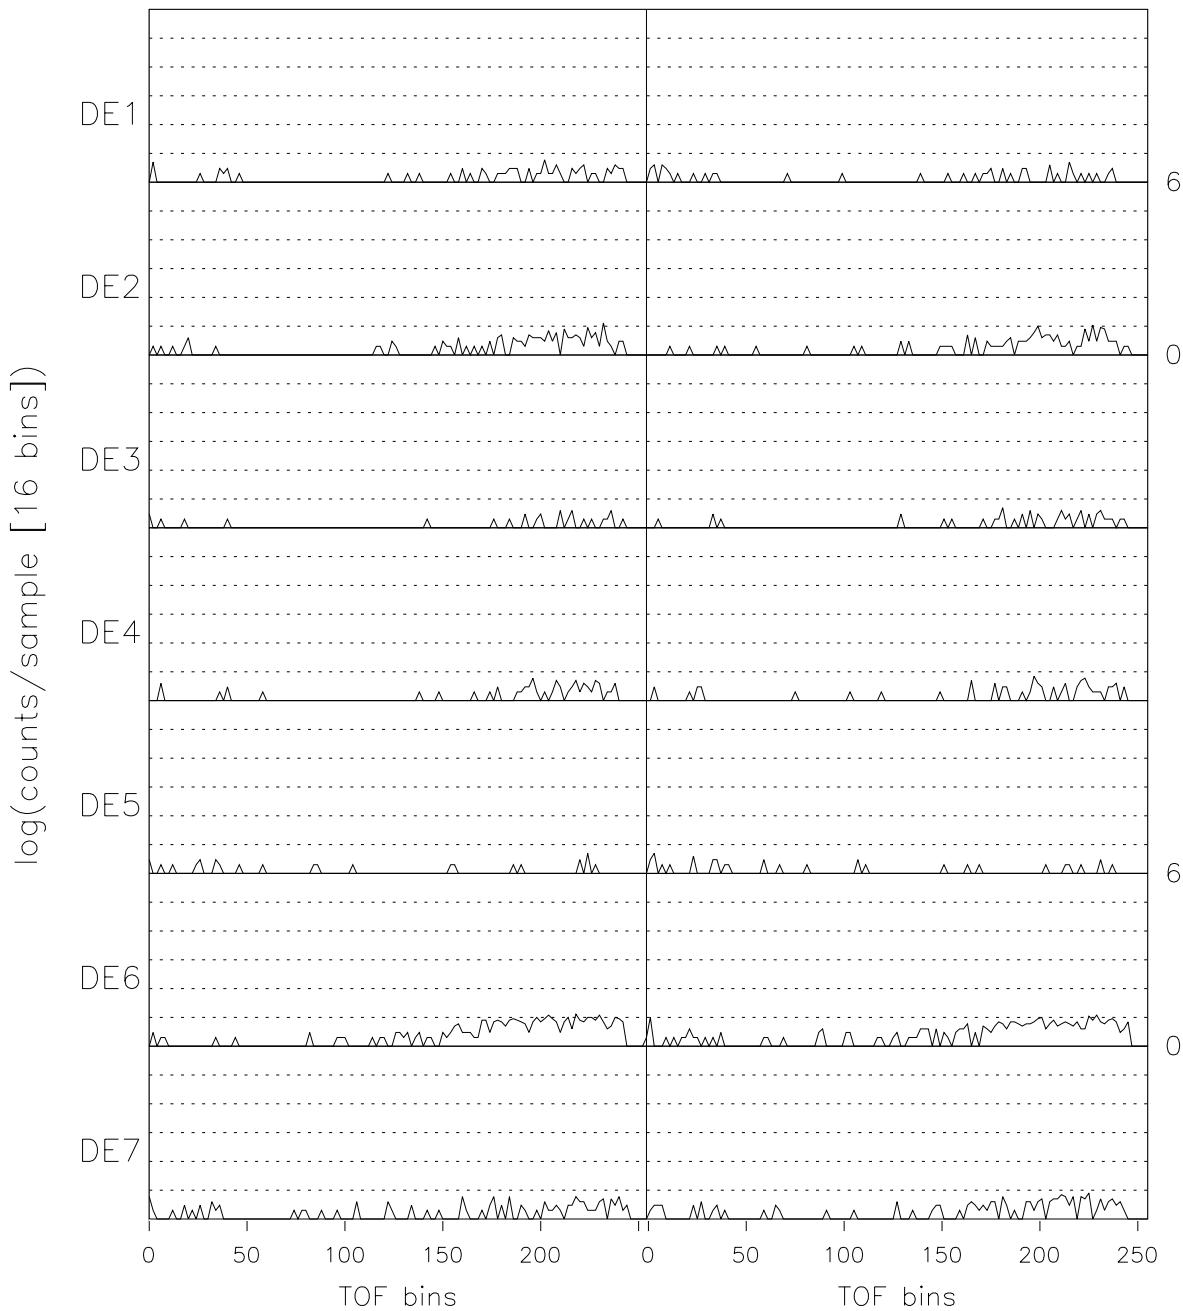

reported: 11-05-06 03:26:18 UT

reported: 11-05-06 03:29:30 UT

file: /export/data/tide/nrt/06110501.dat

-15kV TOF: -9245 v  
-3.6kV MCP: -3364 v  
-2.4kV MCP: -1774 v  
Input Cur: 310 ma  
RPA max: 238 v  
Mirror max: 238 v